

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name D:\Data\Mass Spectrometry Service\77493-000001.d
Method SM MS 50 to 600.m
Sample Name Harkiss-AHH059
Comment

Acquisition Date 5/4/2021 12:10:00 PM

Operator user
Instrument / Ser# micrOTOF-Q 74

Acquisition Parameter

Source Type ESI Ion Polarity Positive
Scan Begin 50 m/z
Scan End 600 m/z

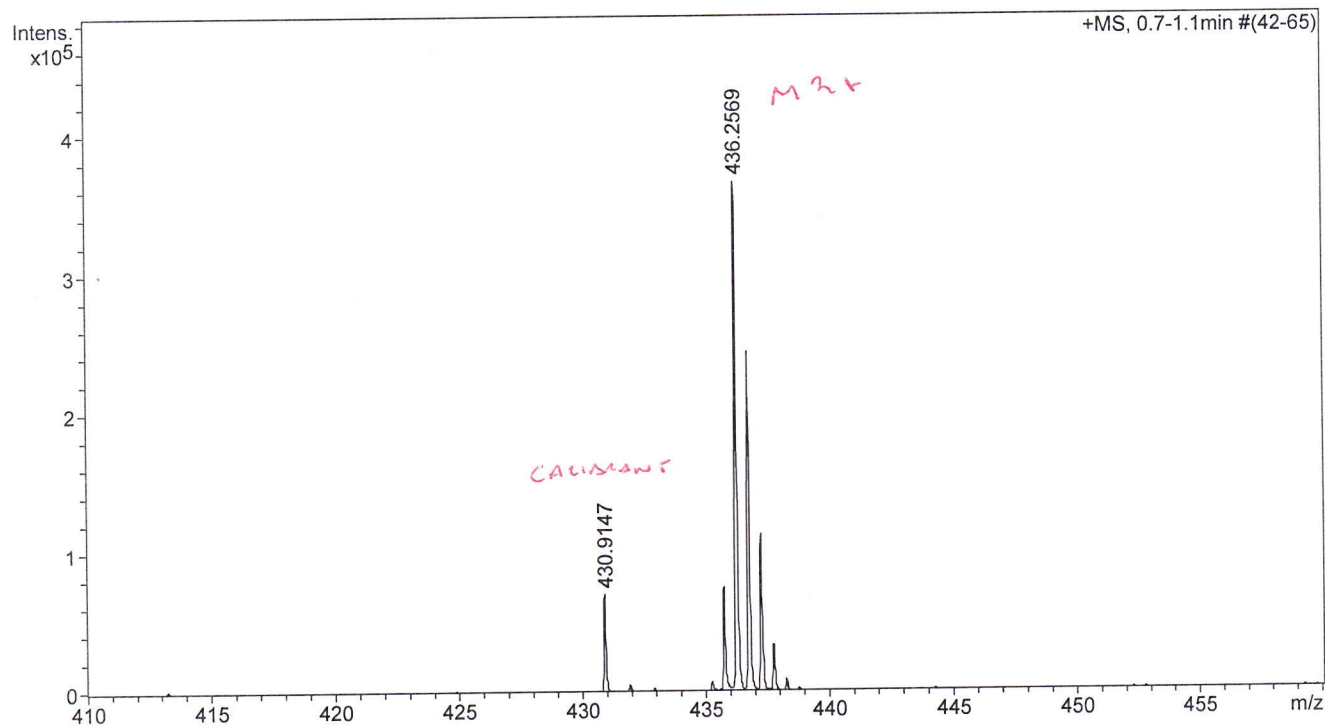

Formula	z	m/z	Meas. m/z	err [ppm]	err [mDa]
C 50 H 26 D 30 N 2 O 2 P 2 S 2	2+	436.2565	436.2569	-0.8	-0.4