

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name D:\Data\Mass Spectrometry Service\77309-000001.d
Method SM MS 50 to 600.m
Sample Name Harkiss-AHH049
Comment

Acquisition Date 4/8/2021 2:34:27 PM

Operator user
Instrument / Ser# micrOTOF-Q 74

Acquisition Parameter

Source Type ESI Ion Polarity Positive
Scan Begin 50 m/z
Scan End 600 m/z

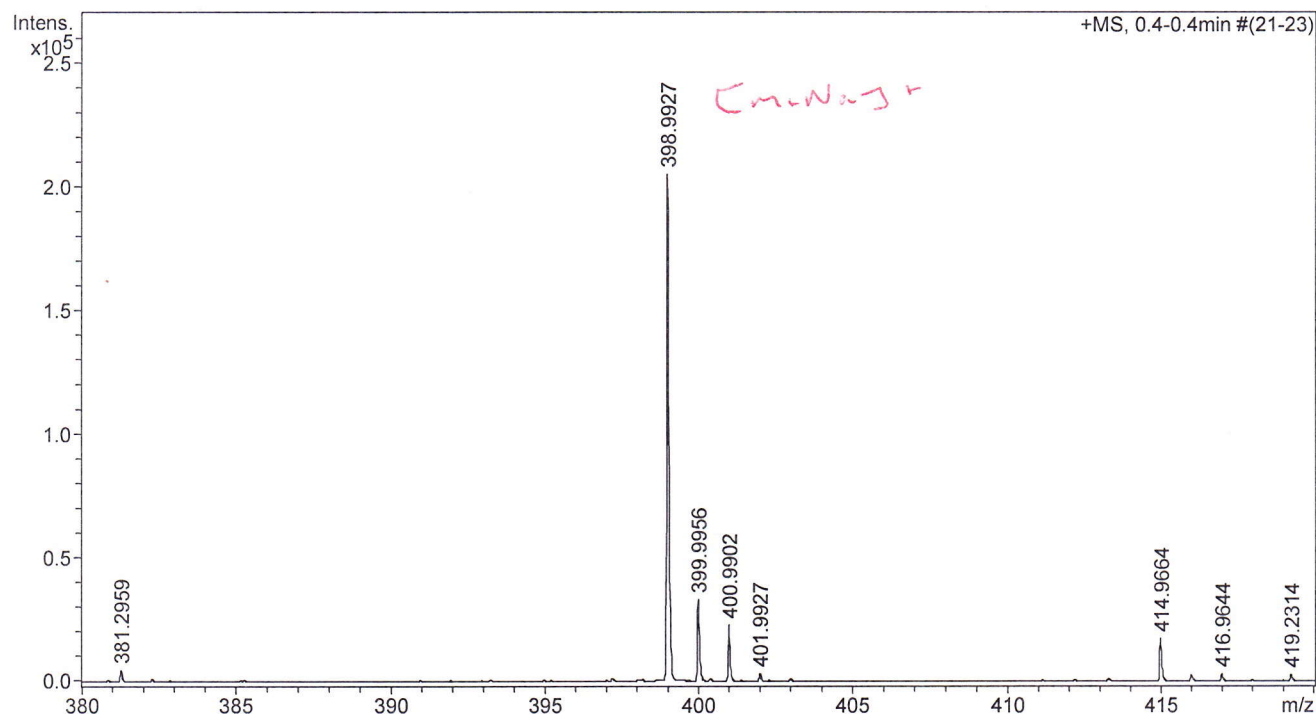

Formula	z	m/z	Meas. m/z	err [ppm]	err [mDa]
C ₁₂ H ₁₂ N ₂ NaO ₈ S ₂	1+	398.9927	398.9927	0.0	0.0