

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name D:\Data\Mass Spectrometry Service\77347-000002.d
Method SM MS 50 to 600.m
Sample Name Harkiss-AHH051
Comment

Acquisition Date 4/14/2021 11:15:48 AM

Operator user
Instrument / Ser# micrOTOF-Q 74

Acquisition Parameter

Source Type ESI Ion Polarity Positive
Scan Begin 50 m/z
Scan End 600 m/z

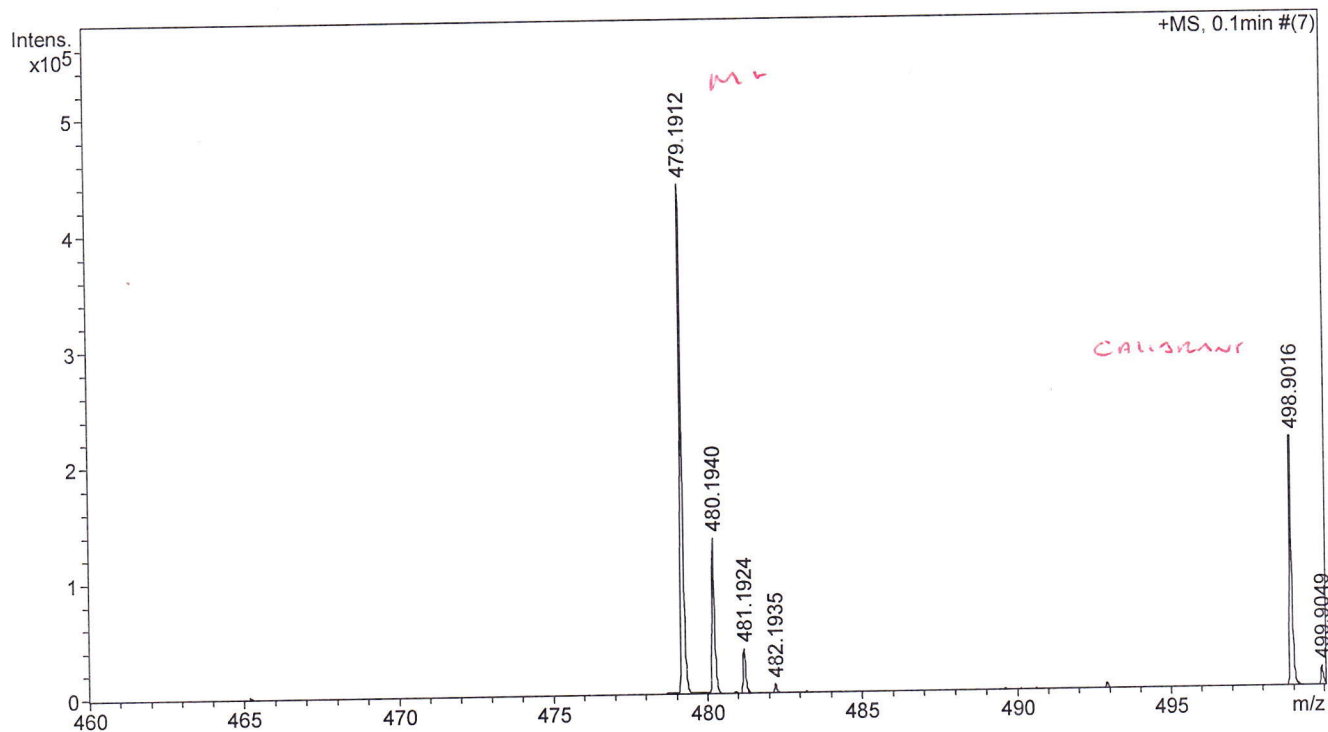

| Formula | z | m/z | Meas. m/z | err [ppm] | err [mDa] |
|-----------------------|----|----------|-----------|-----------|-----------|
| C 27 H 32 N 2 O 2 P S | 1+ | 479.1917 | 479.1912 | 0.9 | 0.5 |