

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name D:\Data\Mass Spectrometry Service\77509-000001.d
Method SM MS 50 to 600.m
Sample Name Harkiss-AHH061
Comment

Acquisition Date 5/5/2021 2:29:54 PM

Operator user
Instrument / Ser# micrOTOF-Q 74

Acquisition Parameter

Source Type ESI Ion Polarity Positive
Scan Begin 50 m/z
Scan End 600 m/z

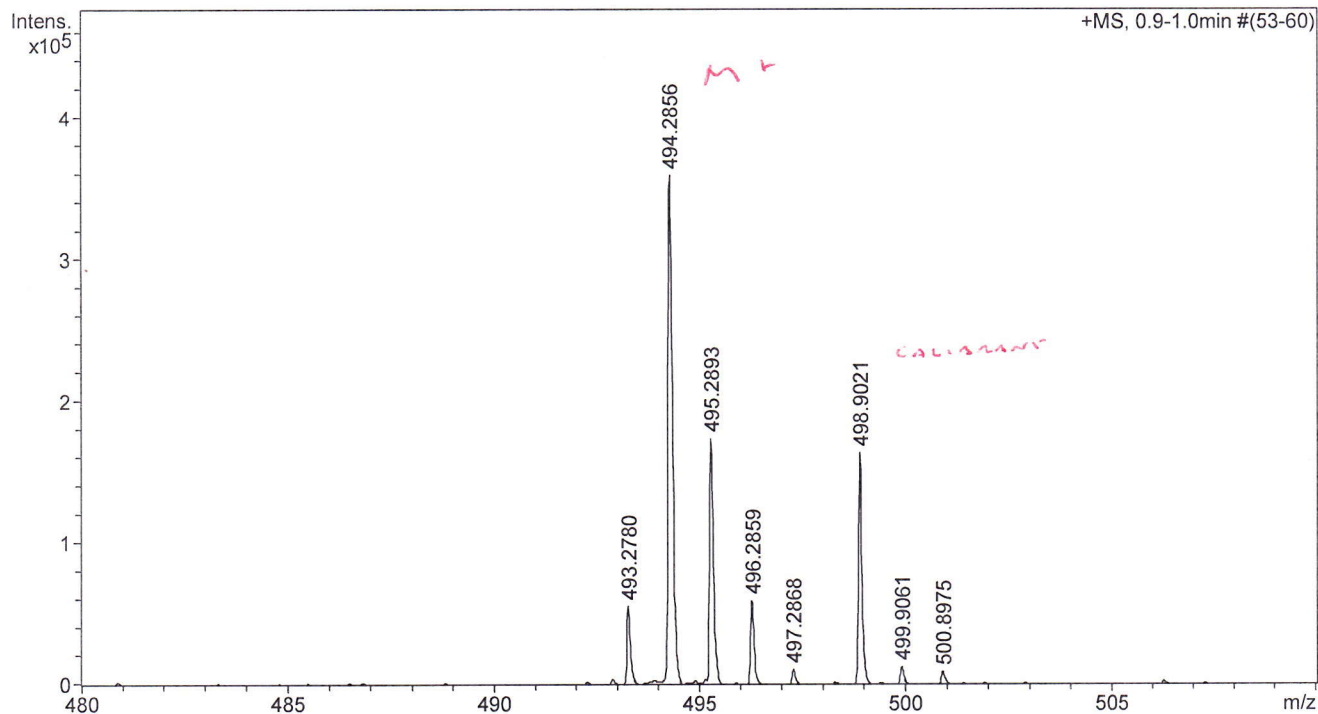

Formula	z	m/z	Meas. m/z	err [ppm]	err [mDa]
C 27 H 17 D 15 N 2 O 2 P S	1+	494.2858	494.2856	0.4	0.2