

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name D:\Data\Mass Spectrometry Service\76415-000001.d
Method SM MS 50 to 600.m
Sample Name Warrington-SW-114
Comment

Acquisition Date 11/5/2020 12:45:11 PM

Operator user
Instrument / Ser# micrOTOF-Q 74

Acquisition Parameter

Source Type ESI Ion Polarity Positive
Scan Begin 50 m/z
Scan End 600 m/z

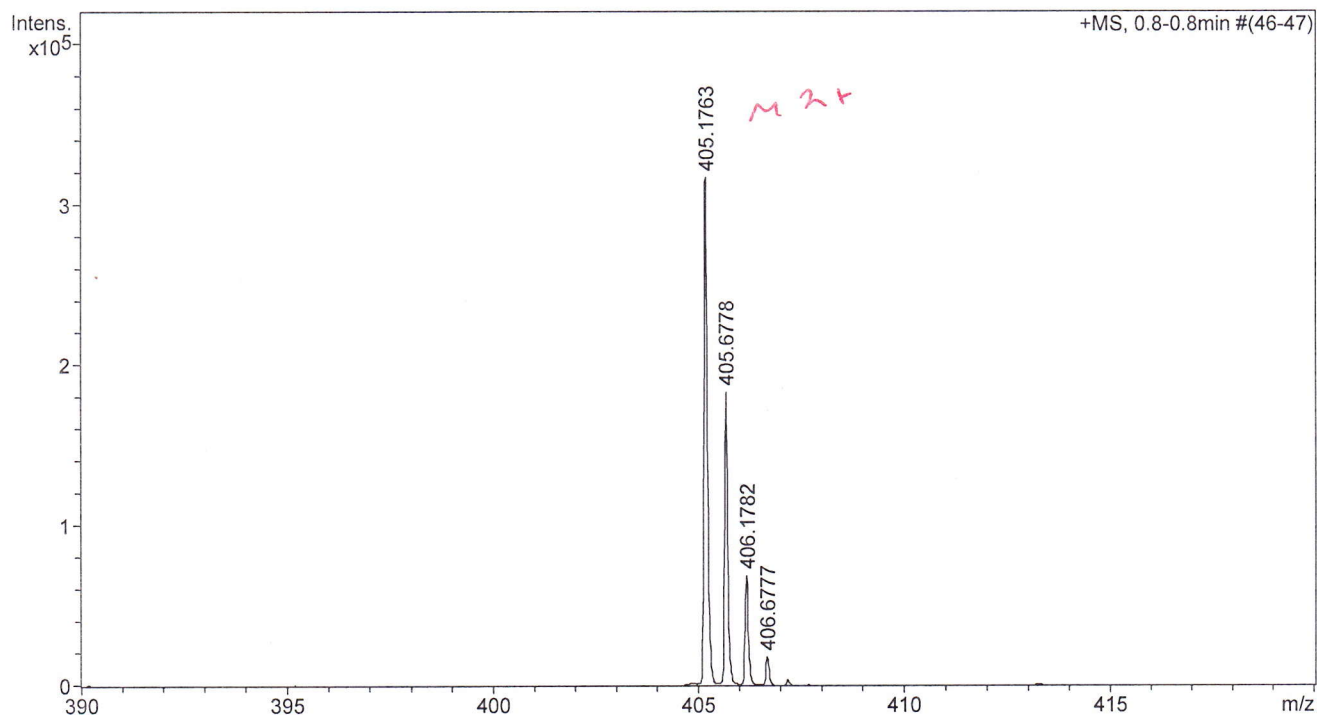

Formula	z	m/z	Meas. m/z	err [ppm]	err [mDa]
C 50 H 56 N 2 O 2 P 2 S	2+	405.1763	405.1763	0.1	0.0