

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name D:\Data\Mass Spectrometry Service\77345-000001.d
Method SM MS 50 to 600.m
Sample Name Harkiss-AHH050
Comment

Acquisition Date 4/13/2021 2:59:49 PM

Operator user
Instrument / Ser# micrOTOF-Q 74

Acquisition Parameter

Source Type ESI Ion Polarity Positive
Scan Begin 50 m/z
Scan End 600 m/z

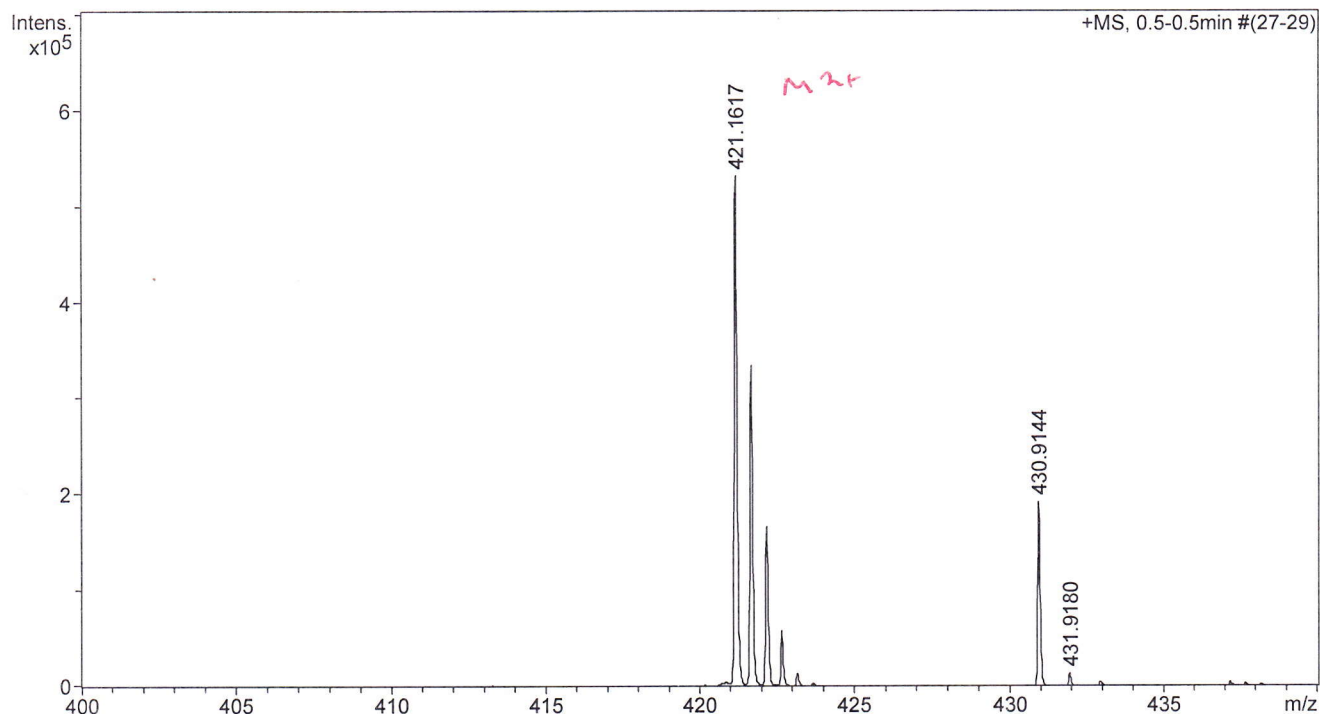

Formula	z	m/z	Meas. m/z	err [ppm]	err [mDa]
C ₅₀ H ₅₆ N ₂ O ₂ P ₂ S ₂	2+	421.1624	421.1617	1.5	0.6