


SC-15-84P



Current Data Parameters
NAME SC-15-84P
EXPNO 15
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240420
Time 14.41 h
INSTRUM spect
PROBHD Z116098_0527 (
PULPROG zg30
TD 261896
SOLVENT MeOD
NS 16
DS 0
SWH 125000.000 Hz
FIDRES 0.954577 Hz
AQ 1.0475841 sec
RG 212.93
DW 4.000 usec
DE 7.15 usec
TE 298.2 K
D1 1.00000000 sec
TD0 1
SFO1 376.5548024 MHz
NUC1 19F
P0 6.00 usec
P1 18.00 usec
PLW1 15.94799995 W

F2 - Processing parameters
SI 262144
SF 376.5924602 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 2.00

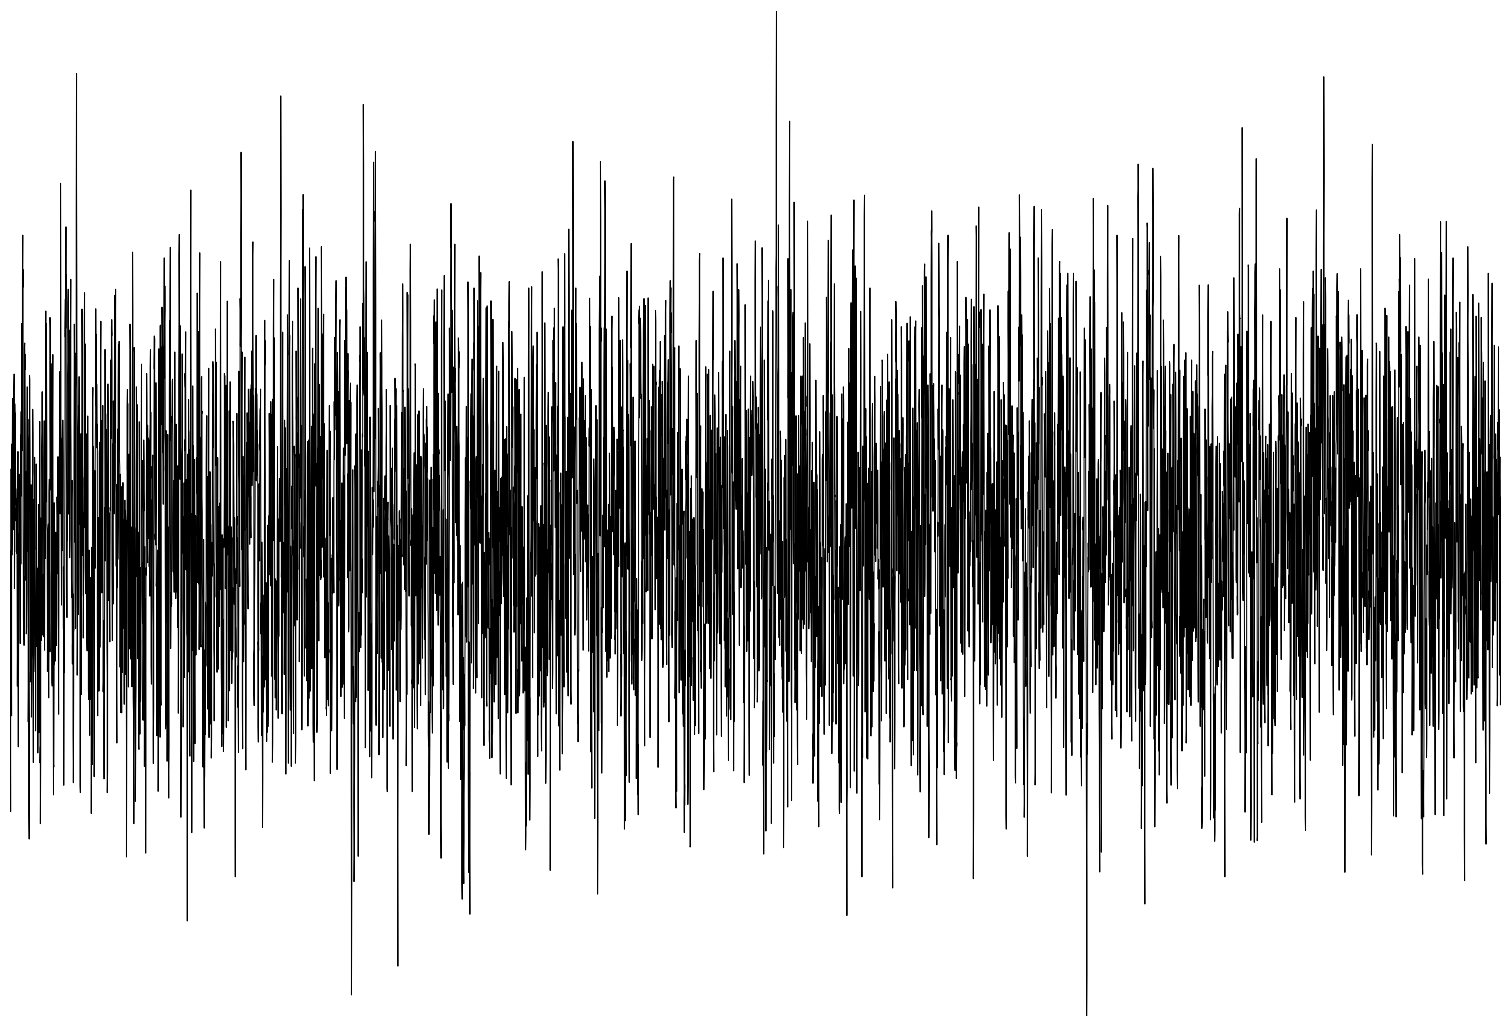

-137 -138 -139 -140 -141 -142 -143 -144 -145 -146 -147 -148 -149 ppm