


SC-15-85P



Current Data Parameters  
NAME SC-15-85P  
EXPNO 12  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20240423  
Time 9.05 h  
INSTRUM spect  
PROBHD Z116098\_0025 (  
PULPROG zgig30  
TD 261896  
SOLVENT MeOD  
NS 16  
DS 4  
SWH 150000.000 Hz  
FIDRES 1.145493 Hz  
AQ 0.8729867 sec  
RG 208.37  
DW 3.333 usec  
DE 6.53 usec  
TE 300.2 K  
D1 1.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 376.4607178 MHz  
NUC1 19F  
P0 4.67 usec  
P1 14.00 usec  
PLW1 20.47699928 W  
SFO2 400.1316005 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 16.15699959 W  
PLW12 0.19550000 W

F2 - Processing parameters  
SI 262144  
SF 376.4983662 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 2.00

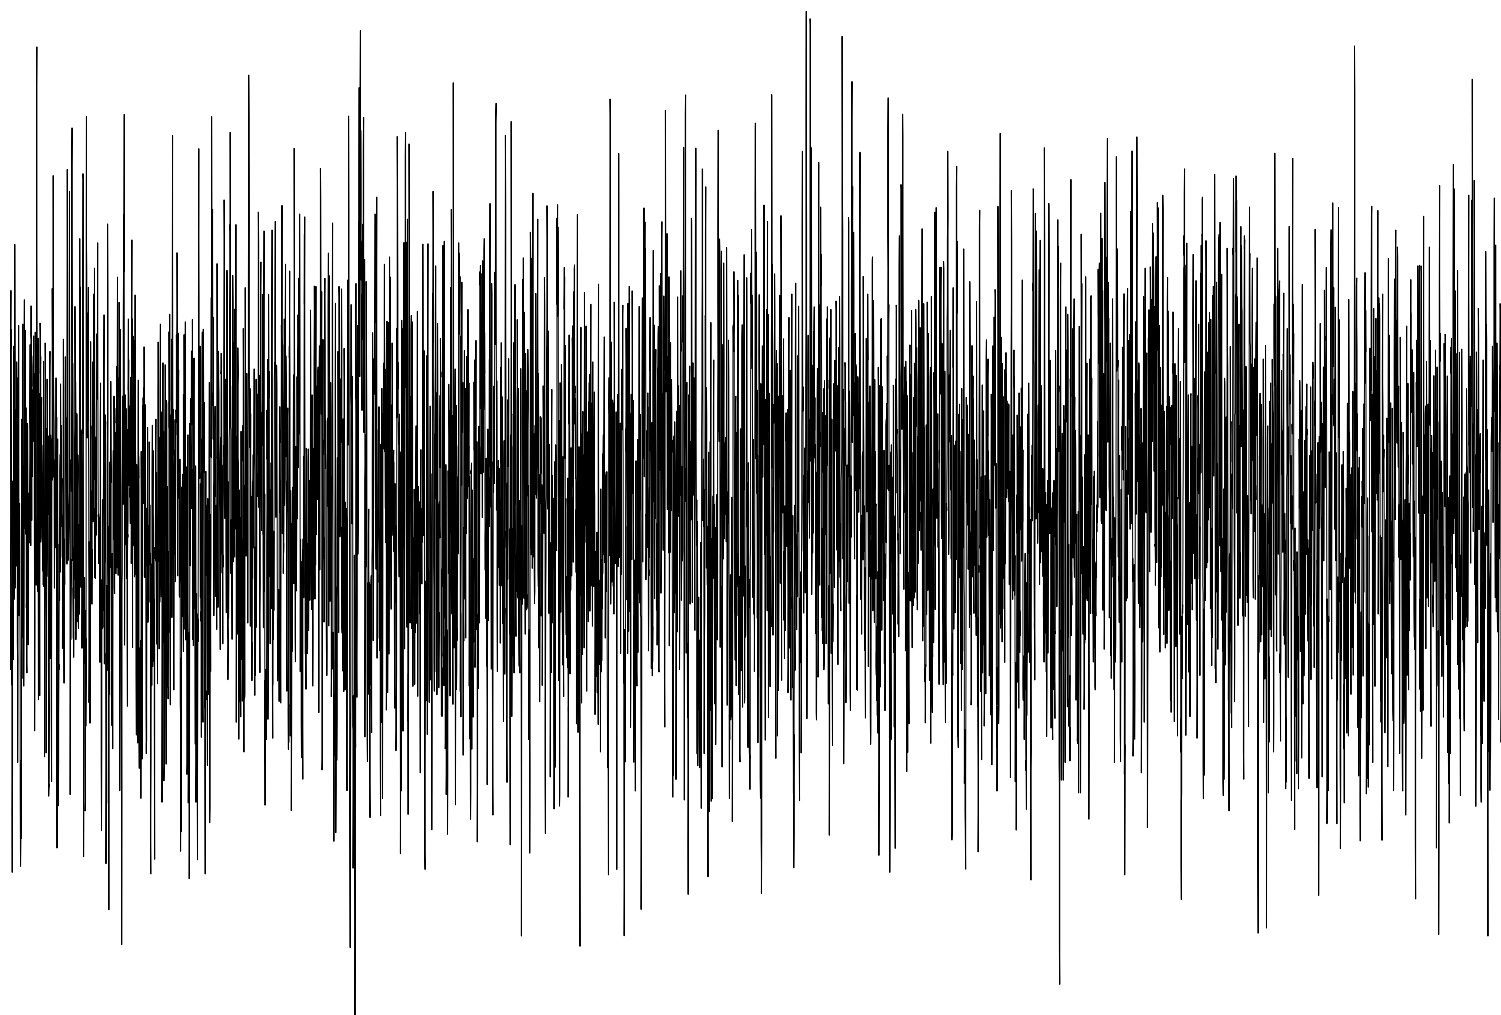

-137 -138 -139 -140 -141 -142 -143 -144 -145 -146 -147 -148 -149 ppm