


SC-15-85P



Current Data Parameters
NAME SC-15-85P2
EXPNO 16
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240424
Time 1.24 h
INSTRUM spect
PROBHD Z116098_0025 (
PULPROG zg30
TD 261896
SOLVENT MeOD
NS 16
DS 0
SWH 150000.000 Hz
FIDRES 1.145493 Hz
AQ 0.8729867 sec
RG 208.37
DW 3.333 usec
DE 6.53 usec
TE 300.2 K
D1 1.00000000 sec
TD0 1
SFO1 376.4607178 MHz
NUC1 19F
P0 4.67 usec
P1 14.00 usec
PLW1 20.47699928 W

F2 - Processing parameters
SI 262144
SF 376.4983662 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 2.00

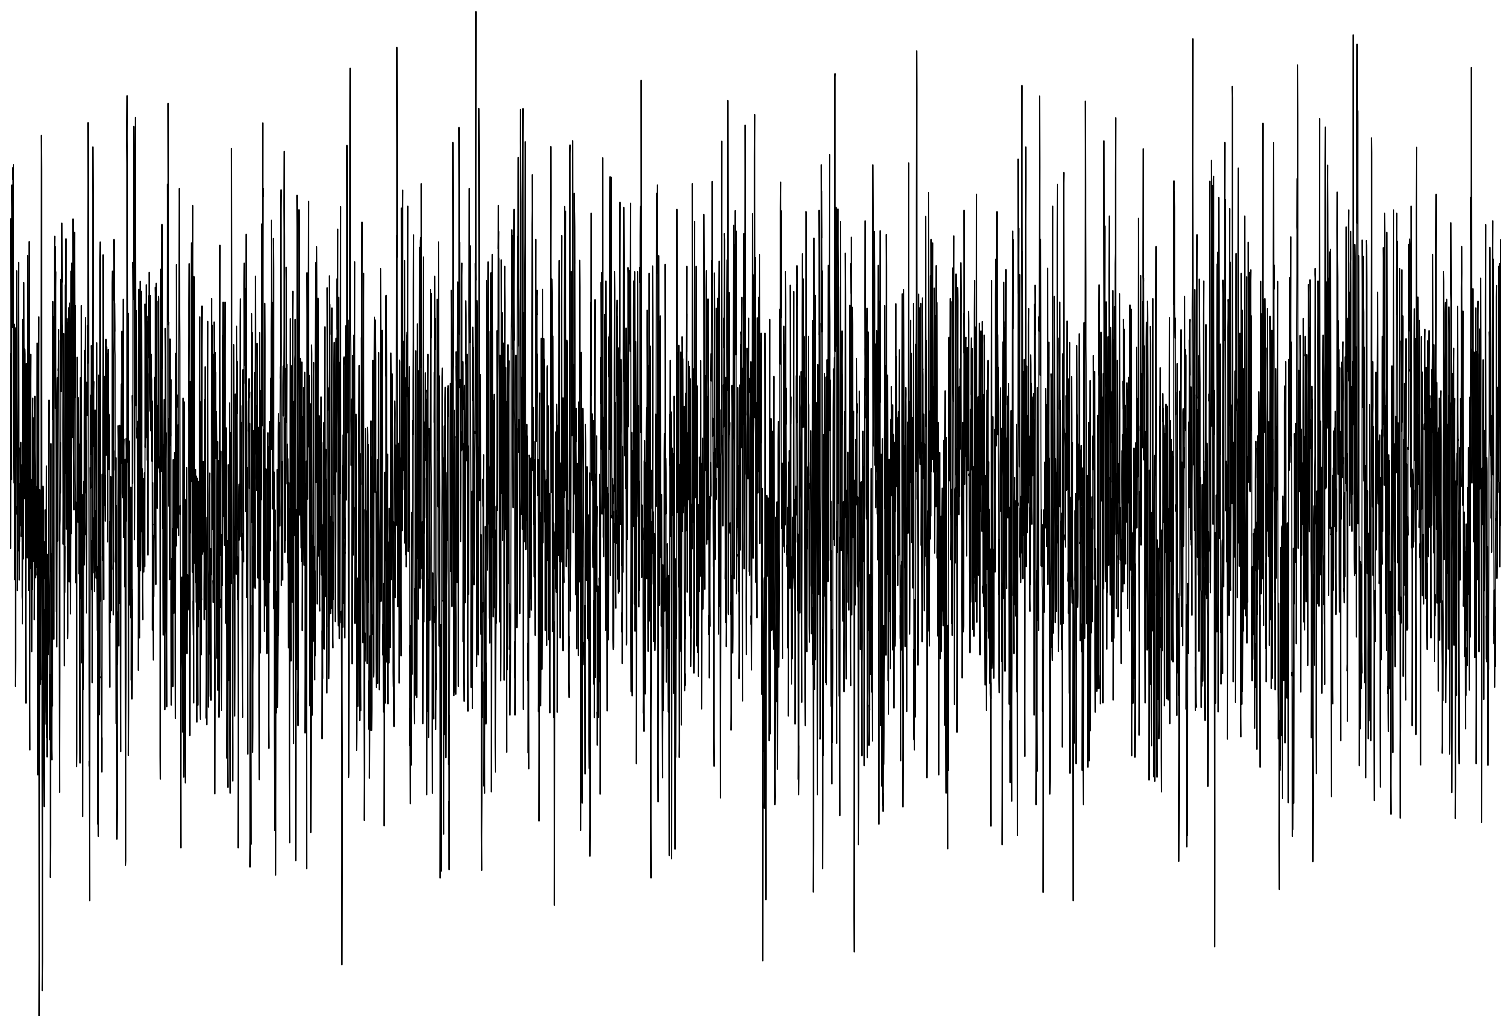

-137 -138 -139 -140 -141 -142 -143 -144 -145 -146 -147 -148 -149 ppm