


SC-9-50P2

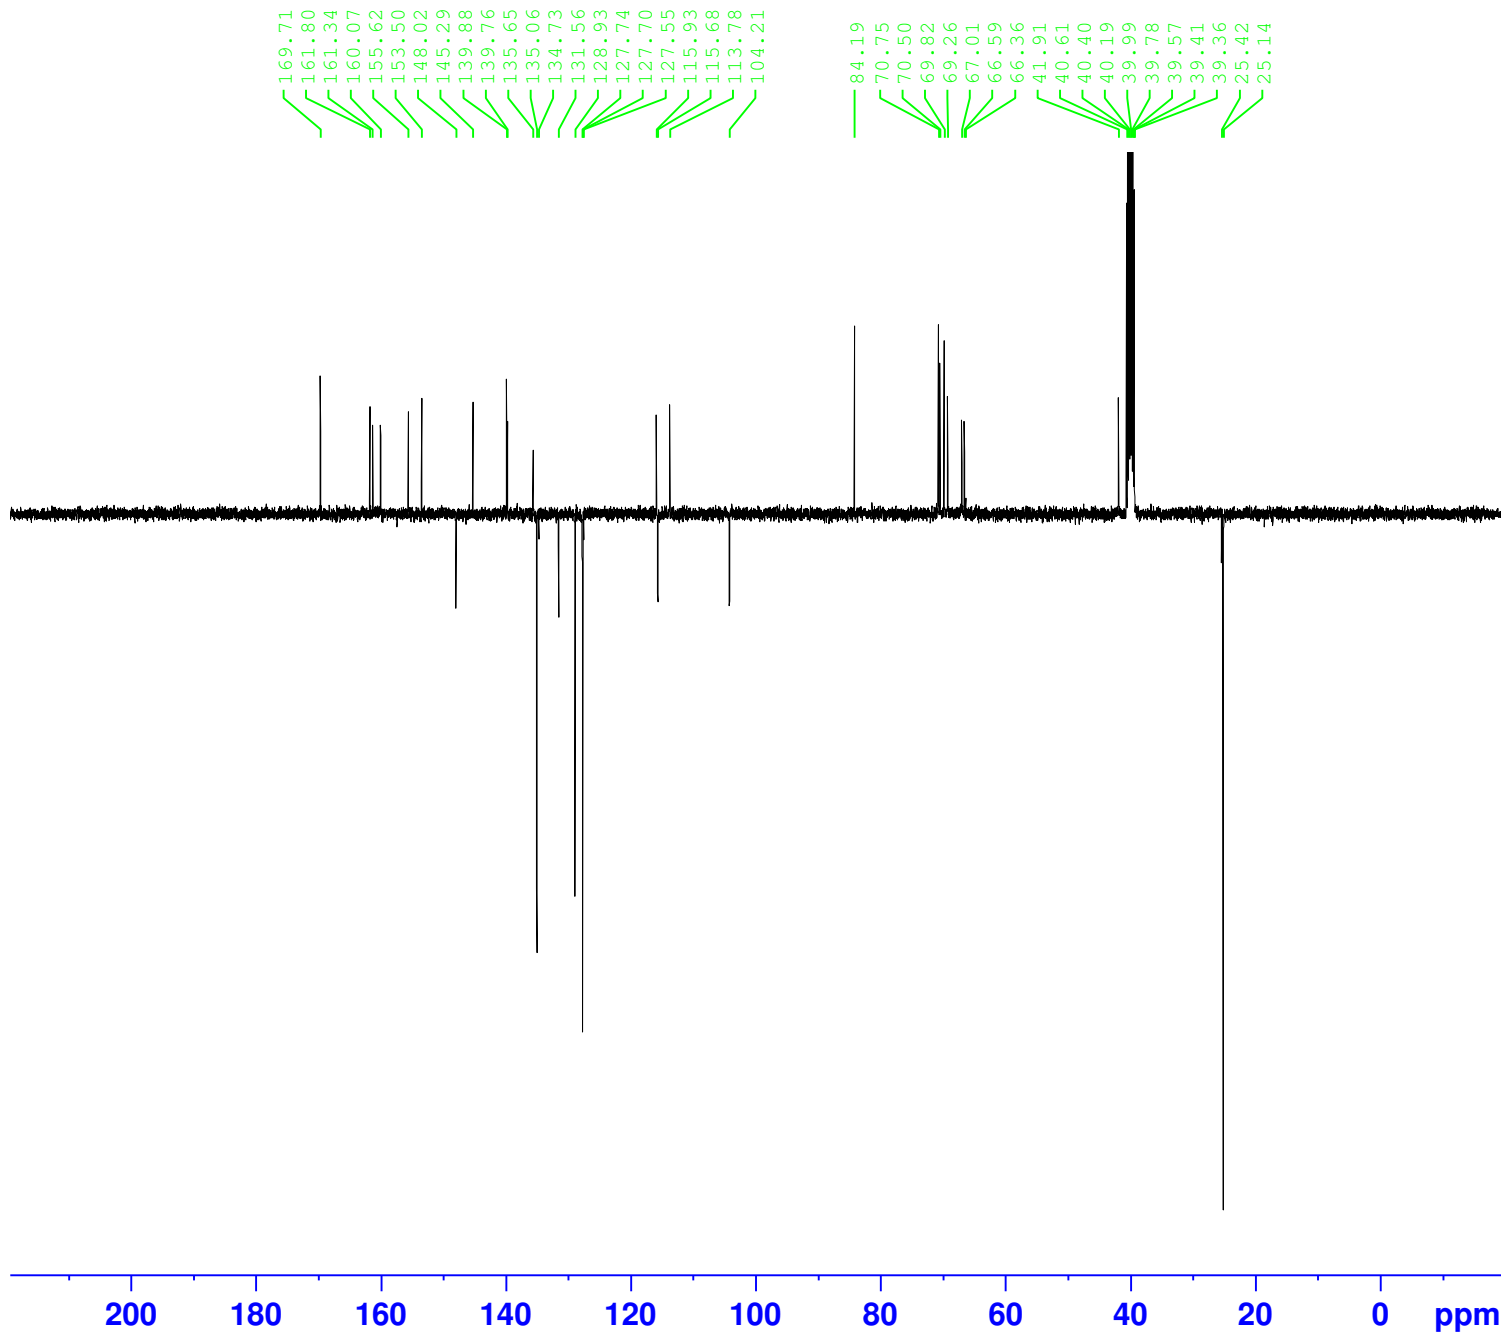

Current Data Parameters
NAME SC-9-50P2
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230202
Time 23.50 h
INSTRUM spect
PROBHD Z116098_0527 (
PULPROG jmod
TD 65536
SOLVENT DMSO
NS 4000
DS 4
SWH 24038.461 Hz
FIDRES 0.733596 Hz
AQ 1.3631488 sec
RG 212.93
DW 20.800 usec
DE 6.50 usec
TE 298.2 K
CNST2 145.000000
CNST11 1.000000
D1 2.00000000 sec
D20 0.00689655 sec
TD0 1
SFO1 100.6479773 MHz
NUC1 13C
P1 10.00 usec
P2 20.00 usec
PLW1 80.98200226 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 16.02700043 W
PLW12 0.19786000 W

F2 - Processing parameters
SI 32768
SF 100.6379135 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40